

SVENSK STANDARD

SS 8760013:2017

Fastställt/Approved: 2017-11-09
Utgåva/Edition: 2
Språk/Language: engelska/English
ICS: 11.140



Sjukvårdstextilier – Bestämning av kontaktryck hos madrasser, sängar och andra liggunderlag

Health care textiles – Determination of contact pressure on mattresses, beds and other underlay



Standarder får världen att fungera

SIS (Swedish Standards Institute) är en fristående ideell förening med medlemmar från både privat och offentlig sektor. Vi är en del av det europeiska och globala nätverk som utarbetar internationella standarder. Standarder är dokumenterad kunskap utvecklad av framstående aktörer inom industri, näringsliv och samhälle och befrämjar handel över gränser, bidrar till att processer och produkter blir säkrare samt effektiviserar din verksamhet.

Delta och påverka

Som medlem i SIS har du möjlighet att påverka framtida standarder inom ditt område på nationell, europeisk och global nivå. Du får samtidigt tillgång till tidig information om utvecklingen inom din bransch.

Ta del av det färdiga arbetet

Vi erbjuder våra kunder allt som rör standarder och deras tillämpning. Hos oss kan du köpa alla publikationer du behöver – allt från enskilda standarder, tekniska rapporter och standardpaket till handböcker och onlinetjänster. Genom vår webbtjänst e-nav får du tillgång till ett lättnavigerat bibliotek där alla standarder som är aktuella för ditt företag finns tillgängliga. Standarder och handböcker är källor till kunskap. Vi säljer dem.

Utveckla din kompetens och lyckas bättre i ditt arbete

Hos SIS kan du gå öppna eller företagsinterna utbildningar kring innehåll och tillämpning av standarder. Genom vår närhet till den internationella utvecklingen och ISO får du rätt kunskap i rätt tid, direkt från källan. Med vår kunskap om standarders möjligheter hjälper vi våra kunder att skapa verklig nytta och lönsamhet i sina verksamheter.

Vill du veta mer om SIS eller hur standarder kan effektivisera din verksamhet är du välkommen in på www.sis.se eller ta kontakt med oss på tel 08-555 523 00.



Standards make the world go round

SIS (Swedish Standards Institute) is an independent non-profit organisation with members from both the private and public sectors. We are part of the European and global network that draws up international standards. Standards consist of documented knowledge developed by prominent actors within the industry, business world and society. They promote cross-border trade, they help to make processes and products safer and they streamline your organisation.

Take part and have influence

As a member of SIS you will have the possibility to participate in standardization activities on national, European and global level. The membership in SIS will give you the opportunity to influence future standards and gain access to early stage information about developments within your field.

Get to know the finished work

We offer our customers everything in connection with standards and their application. You can purchase all the publications you need from us - everything from individual standards, technical reports and standard packages through to manuals and online services. Our web service e-nav gives you access to an easy-to-navigate library where all standards that are relevant to your company are available. Standards and manuals are sources of knowledge. We sell them.

Increase understanding and improve perception

With SIS you can undergo either shared or in-house training in the content and application of standards. Thanks to our proximity to international development and ISO you receive the right knowledge at the right time, direct from the source. With our knowledge about the potential of standards, we assist our customers in creating tangible benefit and profitability in their organisations.

If you want to know more about SIS, or how standards can streamline your organisation, please visit www.sis.se or contact us on phone +46 (0)8-555 523 00



Denna standard fastställdes 2017-11-09 som SS 8760013:2017 och har utgivits i svensk språkversion. Detta dokument återger SS 8760013:2017 i engelsk språkversion. De båda språkversionerna gäller parallellt.

Denna standard ersätter SS 8760013:2010, utgåva 1.

This Standard was approved and published 2017-11-09 as SS 8760013:2017 in Swedish. This document contains an English language version of SS 8760013:2017. The two versions are valid in parallel.

This standard supersedes the Swedish Standard SS 8760013:2010, edition 1.

© Copyright/Upphovsrätten till denna produkt tillhör SIS, Swedish Standards Institute, Stockholm, Sverige. Användningen av denna produkt regleras av slutanvändarlicensen som återfinns i denna produkt, se standardens sista sidor.

© Copyright SIS, Swedish Standards Institute, Stockholm, Sweden. All rights reserved. The use of this product is governed by the end-user licence for this product. You will find the licence in the end of this document.

Uppllysningar om sakinnehållet i standarden lämnas av SIS, Swedish Standards Institute, telefon 08-555 520 00. Standarder kan beställas hos SIS som även lämnar allmänna uppllysningar om svensk och utländsk standard.

Information about the content of the standard is available from the Swedish Standards Institute (SIS), telephone +46 8 555 520 00. Standards may be ordered from SIS, who can also provide general information about Swedish and foreign standards.

Denna standard är framtagen av kommittén för Trycksårsprevention, SIS/TK 595.

Har du synpunkter på innehållet i den här standarden, vill du delta i ett kommande revideringsarbete eller vara med och ta fram andra standarder inom området? Gå in på www.sis.se - där hittar du mer information.

Contents

Page

Introduction	3
1 Scope	4
2 Terms and definitions	4
3 Equipment	4
3.1 Pressure sensing mat	4
3.2 Large indenter.....	4
3.3 Small indenter.....	5
4 Conditioning and testing climate.....	6
5 Testing procedure	6
5.1 Overview.....	6
5.2 Test objects.....	6
5.3 Measuring positions.....	6
5.4 Pressure measurements and control of indentation depth	7
6 Calculations	7
6.1 Maximum pressure for large indenter	7
6.2 Maximum pressure for small indenter	7
7 Test report.....	8
Bibliography.....	9

Introduction

This standard contains a method for determining the pressure distribution properties of an underlay. This is done by measuring the pressure distribution on the contact surface between the underlay and indenters, which simulate various parts of the human body. The maximum pressure that occurs on a contact surface of this type is affected by the nature of the underlay and is considered to be a good measure of its pressure distribution capabilities. The lower the maximum pressure, the better the pressure distribution capability.

The underlay, as defined in this standard, may comprise one or more components. The test method is based on a simplification of actual conditions (in respect of the geometry of the indenters, for example). This means that the maximum pressures (absolute values) measured may deviate from those occurring in an actual situation, when a person is lying on a bed. The extent of this deviation may vary depending on anthropometrics and the type of mattress, for example. However, measuring according to this method is considered to provide reliable information regarding which of a number of different underlays best distributes the pressure from a human body.

Edition 2 differs from edition 1 due to updating and clarification of the text, plus the addition of an explanatory section for information purposes.

The standard provides no guidance on the selection of mattresses or other types of underlay. Please see SS 8760020 for issues relating to requirements for care mattresses.

1 Scope

This standard describes a method for determining the pressure distribution capability of an underlay by measuring the contact pressure between indenters that simulate various parts of the human body, and the underlay. The underlay may comprise one or more components.

The test method as described in this standard can be used when testing new, used and/or aged underlays.

This test method is not intended for testing air mattresses, water mattresses or similar products.

2 Terms and definitions

The terms and definitions that follow below are applicable to application of this document.

- 2.1
pressure distribution**
pressure variation over a given test area
- 2.2
underlay**
one or more separate mattress layers with or without encasing, plus other components that affect the distribution of the pressure
- 2.3
pressure sensing mat**
a thin, formable mat with measurement cells distributed over the surface in a grid pattern.

Note 1 to entry Measurement cells record contact pressure

3 Equipment

3.1 Pressure sensing mat

The pressure sensing mat shall have an effective measurement area of at least 40 cm × 40 cm.

To achieve sufficiently good dissolution of the distribution of the pressure, individual measurement cells in the pressure sensing mat shall be no larger than 20 mm × 20 mm.

The pressure sensing mat shall come with a unit for collecting measurement values, facilitating measurement at specific times. The unit shall facilitate subsequent evaluation of the pressure values of individual measurement cells.

The pressure sensing mat shall have a measurement accuracy of a maximum of $\pm 10\%$.

3.2 Large indenter

A large indenter shall be rigid, smooth and rotationally symmetrical, and superelliptical with a radius (R) of 20 cm and height (H) of 12 cm.

Note 1: Aluminium is an example of an appropriate material for the indenter.

The shape of the indenter, which is designed to simulate the shape of the back and bottom of an "average" man, can be described mathematically using the following formula:

$$\frac{X^2}{R^2} + \frac{Y^2}{R^2} + \frac{Z^3}{H^3} = 1$$

Where X and Y state the position laterally in cm Z states the position vertically in cm.

A large indenter shall, for the loading case normal load, exert a force of (300 ± 5) N when placed on an underlay.

Note 2: Normal load indicates approximately the pressure on a normal foam mattress that is achieved when a person weighing 80 kg to 90 kg is lying on his/her back on the same mattress.

A large indenter shall also be able to exert the force (600 ± 10) N when it is placed on an underlay. This load case is referred to as elevated load and shall, for example, simulate the load from heavier individuals when turning, sitting on the bed or lying on their sides.

The indenter shall maintain a temperature of (34 ± 2) °C during testing.

3.3 Small indenter

A small indenter shall be rigid, smooth, rotationally symmetrical, and superelliptical. It shall have a radius (R) of 6 cm and height (H) of 4.5 cm.

A small indenter shall exert a force of (40 ± 1) N when placed on an underlay. This load case shall represent small body parts (knees, elbows and heels) and can be described mathematically using the formula in 3.2.

The indenter shall maintain a temperature of (34 ± 2) °C during testing.

Note: Figure 1 shows examples of appropriate indenters.



Figure 1 – Examples of large and small indenters

SS 8760013:2017 (En)**4 Conditioning and testing climate**

Prior to a testing procedure, the test objects (underlay) shall have been stored indoors for at least 72 h and conditioned in the testing climate (50 ± 5) % relative humidity at (23 ± 2) °C for at least 24 h. During this time, the test objects shall be stored so that they are not subjected to mechanical load.

5 Testing procedure**5.1 Overview**

Use the three load cases during the testing procedure. The indenters simulate various selected and relevant loads from a person lying on the underlay. Perform measurements at five measuring positions on each underlay.

Measure the contact pressure occurring when each of the three indenters is pressed against the underlay, using an intermediate pressure sensing mat. The pressure varies at different locations on the contact surface.

Select the maximum pressure recorded by the pressure sensing mat as output data. The maximum pressure is considered to be a good measure of the pressure distribution capability of an underlay (the lower the maximum pressure, the better the pressure distribution). Three maximum pressures (one from each load case) will therefore be determined at each measuring position.

Also use one of the indenters for measuring the indentation depth at each measuring position.

Calculate the average of the measured maximum pressures from the five measuring positions for each indenter. These averages constitute the primary results from the testing procedure. Calculate the average from the five indentation depth measurements and specify these in the report as well.

5.2 Test objects

The underlays are test objects and may comprise one or more layers; e.g. mattress/bed, mattress pad and sheet. If multiple layers are tested together, they shall be positioned in the way in which they are normally used. Place the test objects on a base that cannot be compressed.

5.3 Measuring positions

There shall be five measuring positions for each load case. To prevent edge effects and oblique loading, the centres of all measuring positions shall, if possible, be located at least 30 cm from the outer edges of the test objects. With these restrictions, the measuring points shall be distributed over the available area.

EXAMPLE: Appropriate positioning of the measuring positions for a test object of dimensions 90 cm × 200 cm is shown in Figure 2. The dashed area shows the zone (30 cm × 140 cm) within which the centre of the indenter is placed.

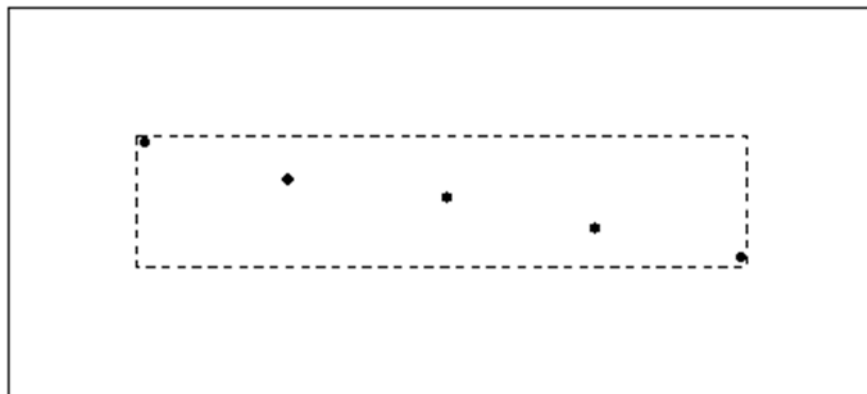


Figure 2 – Example of the positioning of measuring positions