

SVENSK STANDARD

SS-EN ISO 20072:2013



Fastställt/Approved: 2013-06-05
Publicerad/Published: 2013-06-10
Utgåva/Edition: 2
Språk/Language: engelska/English
ICS: 11.040.10

Konstruktion och verifiering av inhalatorer för läkemedelsaerosoler – Krav och provningsmetoder (ISO 20072:2009)

Aerosol drug delivery device design verification – Requirements and test methods (ISO 20072:2009)

This preview is downloaded from www.sis.se. Buy the entire standard via <https://www.sis.se/std-98316>

Standarder får världen att fungera

SIS (Swedish Standards Institute) är en fristående ideell förening med medlemmar från både privat och offentlig sektor. Vi är en del av det europeiska och globala nätverk som utarbetar internationella standarder. Standarder är dokumenterad kunskap utvecklad av framstående aktörer inom industri, näringsliv och samhälle och befrämjar handel över gränser, bidrar till att processer och produkter blir säkrare samt effektiviserar din verksamhet.

Delta och påverka

Som medlem i SIS har du möjlighet att påverka framtida standarder inom ditt område på nationell, europeisk och global nivå. Du får samtidigt tillgång till tidig information om utvecklingen inom din bransch.

Ta del av det färdiga arbetet

Vi erbjuder våra kunder allt som rör standarder och deras tillämpning. Hos oss kan du köpa alla publikationer du behöver – allt från enskilda standarder, tekniska rapporter och standardpaket till handböcker och onlinetjänster. Genom vår webbtjänst e-nav får du tillgång till ett lättnavigerat bibliotek där alla standarder som är aktuella för ditt företag finns tillgängliga. Standarder och handböcker är källor till kunskap. Vi säljer dem.

Utveckla din kompetens och lyckas bättre i ditt arbete

Hos SIS kan du gå öppna eller företagsinterna utbildningar kring innehåll och tillämpning av standarder. Genom vår närhet till den internationella utvecklingen och ISO får du rätt kunskap i rätt tid, direkt från källan. Med vår kunskap om standarders möjligheter hjälper vi våra kunder att skapa verklig nytta och lönsamhet i sina verksamheter.

Vill du veta mer om SIS eller hur standarder kan effektivisera din verksamhet är du välkommen in på www.sis.se eller ta kontakt med oss på tel 08-555 523 00.



Standards make the world go round

SIS (Swedish Standards Institute) is an independent non-profit organisation with members from both the private and public sectors. We are part of the European and global network that draws up international standards. Standards consist of documented knowledge developed by prominent actors within the industry, business world and society. They promote cross-border trade, they help to make processes and products safer and they streamline your organisation.

Take part and have influence

As a member of SIS you will have the possibility to participate in standardization activities on national, European and global level. The membership in SIS will give you the opportunity to influence future standards and gain access to early stage information about developments within your field.

Get to know the finished work

We offer our customers everything in connection with standards and their application. You can purchase all the publications you need from us - everything from individual standards, technical reports and standard packages through to manuals and online services. Our web service e-nav gives you access to an easy-to-navigate library where all standards that are relevant to your company are available. Standards and manuals are sources of knowledge. We sell them.

Increase understanding and improve perception

With SIS you can undergo either shared or in-house training in the content and application of standards. Thanks to our proximity to international development and ISO you receive the right knowledge at the right time, direct from the source. With our knowledge about the potential of standards, we assist our customers in creating tangible benefit and profitability in their organisations.

If you want to know more about SIS, or how standards can streamline your organisation, please visit www.sis.se or contact us on phone +46 (0)8-555 523 00



Europastandarden EN ISO 20072:2013 gäller som svensk standard. Detta dokument innehåller den officiella engelska versionen av EN ISO 20072:2013.

Denna standard ersätter SS-EN ISO 20072:2010, utgåva 1.

The European Standard EN ISO 20072:2013 has the status of a Swedish Standard. This document contains the official version of EN ISO 20072:2013.

This standard supersedes the Swedish Standard SS-EN ISO 20072:2010, edition 1.

© Copyright/Upphovsrätten till denna produkt tillhör SIS, Swedish Standards Institute, Stockholm, Sverige. Användningen av denna produkt regleras av slutanvändarlicensen som återfinns i denna produkt, se standardens sista sidor.

© Copyright SIS, Swedish Standards Institute, Stockholm, Sweden. All rights reserved. The use of this product is governed by the end-user licence for this product. You will find the licence in the end of this document.

Uppllysningar om sakinnehållet i standarden lämnas av SIS, Swedish Standards Institute, telefon 08-555 520 00. Standarder kan beställas hos SIS Förlag AB som även lämnar allmänna uppllysningar om svensk och utländsk standard.

Information about the content of the standard is available from the Swedish Standards Institute (SIS), telephone +46 8 555 520 00. Standards may be ordered from SIS Förlag AB, who can also provide general information about Swedish and foreign standards.

Denna standard är framtagen av kommittén för Förbrukningsmaterial inom sjukvården, SIS/TK 330.

Har du synpunkter på innehållet i den här standarden, vill du delta i ett kommande revideringsarbete eller vara med och ta fram andra standarder inom området? Gå in på www.sis.se - där hittar du mer information.

EUROPEAN STANDARD

EN ISO 20072

NORME EUROPÉENNE

EUROPÄISCHE NORM

February 2013

ICS 11.040.10

Supersedes EN ISO 20072:2010

English Version

Aerosol drug delivery device design verification - Requirements and test methods (ISO 20072:2009)

Vérification de la conception d'un dispositif d'administration
de médicament sous forme d'aérosol - Exigences et
méthodes d'essai (ISO 20072:2009)

Ausführungsverifizierung von Inhalationsgeräten -
Anforderungen und Prüfverfahren (ISO 20072:2009)

This European Standard was approved by CEN on 8 January 2013.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Contents

Page

Foreword.....	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	2
4 Symbols and abbreviated terms	6
5 Requirements	7
5.1 General.....	7
5.2 Risk assessment requirements.....	8
5.3 Device functionality profile.....	8
5.4 System verification test	8
5.5 Uncertainty of measurements and conformance with specification.....	9
5.6 Test requirements.....	9
6 Test methods.....	11
6.1 General.....	11
6.2 Test procedures	12
6.3 Test conditions	16
6.4 Test evaluations.....	17
7 Test report	19
8 Information supplied by the manufacturer	19
8.1 General.....	19
8.2 Marking	19
8.3 Instructions for use	20
Annex A (informative) Rationale for requirements	22
Annex B (informative) Further guidance and clarification of the device functionality profile	24
Annex C (informative) Rationale for test methods.....	26
Annex D (informative) Two-sided tolerance limit factors (<i>k</i>).....	29
Annex E (informative) Alternative acceptance criteria for the device functionality profile evaluation	35
Annex ZA (informative) Relationship between this European Standard and the Essential Requirements of EU Directive 93/42/EEC on Medical Devices.....	42
Bibliography	43

Foreword

The text of ISO 20072:2009 has been prepared by Technical Committee ISO/TC 84 “Devices for administration of medicinal products and intravascular catheters” of the International Organization for Standardization (ISO) and has been taken over as EN ISO 20072:2013 by Technical Committee CEN/TC 205 “Non-active medical devices” the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by August 2013, and conflicting national standards shall be withdrawn at the latest by August 2013.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 20072:2010.

This document has been prepared under a mandate given to CEN by the European Commission and the European Free Trade Association, and supports essential requirements of EU Directive.

For relationship with EU Directive, see informative Annex ZA, which is an integral part of this document.

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Endorsement notice

The text of ISO 20072:2009 has been approved by CEN as EN ISO 20072:2013 without any modification.

Introduction

This International Standard applies to hand-held aerosol drug delivery devices (ADDD) intended to administer medication to humans. To avoid unnecessarily restricting innovation, given the broad variation in device designs, this International Standard addresses the more general design/labelling requirements rather than specific physical and prescriptive design requirements. However, this International Standard does require the elaboration of a device functionality profile (DFP) specific to the ADDD in question. This International Standard also addresses ADDD design requirements from both the user interface and safety perspectives.

An ADDD is used as part of a system consisting of the ADDD, the container, the medication and the labelling, including the instructions for use. Therefore, design verification of the ADDD includes a final system verification test conducted in accordance with the instructions for use.

From a regulatory perspective, the ADDD system may be reviewed and approved as part of a drug product (combination of ADDD and medication) or as a device by itself. For the purposes of this International Standard, such regulatory distinctions do not alter the intent of the design verification process described herein. As an example, in the European Union (EU), if an ADDD is placed on the market in such a way that the ADDD and the medication form a single integral product (i.e. the system) that is intended exclusively for use in the given combination and which is not refillable, that single product shall be governed by Directive 2001/83/EEC. However, the relevant essential requirements of Annex I of the Medical Device Directive (93/42/EEC) shall apply as far as safety and performance-related ADDD features are concerned, which is the specific objective of this design verification standard.

Regardless of the distinctions (“drug” or “device,” pre-filled or refillable), it is recognised that ADDD design verification is an important component of the overall validation process. Moreover, design verification is iterative, to be conducted at various phases throughout the ADDD’s development and subsequent ADDD post-approval modifications. In all instances, design verification is conducted using the phase-appropriate instructions for use. It is understood that in the early phases of ADDD development an appropriate subset of the requirements contained herein might apply, but that all of the requirements will be satisfied as part of the final design verification exercise. Furthermore, design verification should be considered a minimum requirement for the safe and effective use of the ADDD, and in many instances additional testing may be appropriate as indicated by a risk assessment that shall also be conducted.

This International Standard introduces the requirement for developers and/or manufacturers to create a device functionality profile (DFP) for a given ADDD based on the ISO Standard for device risk assessment (as a part of ISO 14971). The device functionality profile defines the parameters and tolerance intervals used to verify the ADDD’s ability to meet the manufacturer’s design specifications during in-use conditions and following environmental and electromechanical extreme use conditions. This International Standard also includes a system verification test conducted at standard atmosphere and nominal flow rate as a simple bridge between the device design and the patient interface.

The purpose of this International Standard is to ensure a method and guide for independent testing of the repeatability and reproducibility of ADDD functionality that verifies compliance with its design specification. The design verification process may include use of applicable regulatory agency requirements and/or test methods. The sampling plans for this International Standard are intended to verify the design at a high confidence level. They do not replace the more general manufacturing quality systems, including lot release, which appear in standards on quality systems (e.g. the ISO 9000 series or ISO 13485).

Figure 1 illustrates the process this International Standard advises to use in order to assess and verify whether a design meets the determined DFP.

SS-EN ISO 20072:2013 (E)

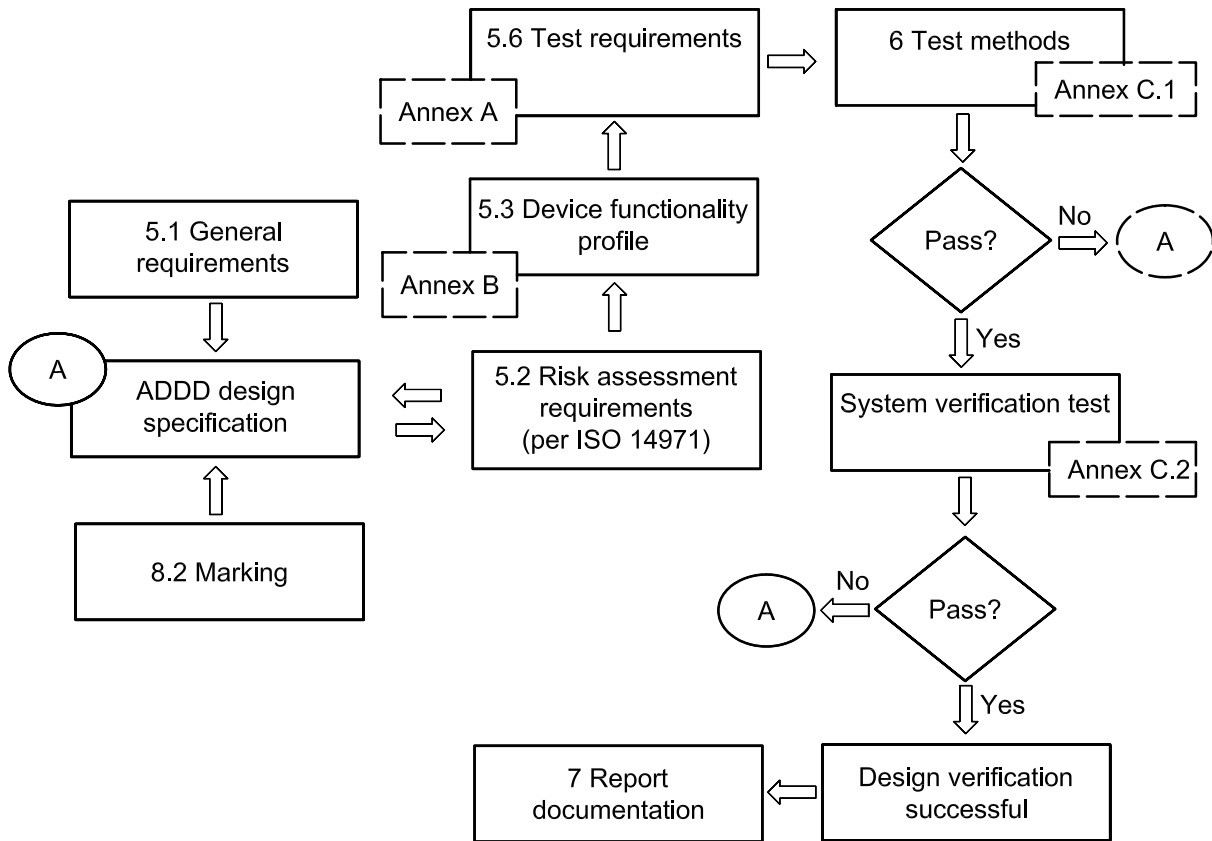


Figure 1 — ADDD design verification process

This International Standard specifically addresses the most basic elements regarding the safe and effective use of ADDD in humans. It does not define the pharmaceutical or clinical performance of an ADDD. Any labelling indicating ADDD use to deliver medication to specific regions of the respiratory tract falls under the authority of national governments or regional agencies regulating the manufacture and marketing of medical devices and pharmaceutical products. In some countries national regulations exist, and their requirements can supersede or complement this International Standard.

For a given manufacturer, existing marketed products and those currently under development might not fulfil some of the requirements. However, manufacturers should comply with this International Standard when improving the functional design of existing ADDDs or developing new ADDDs to obtain an even higher level of quality.

Annex A describes the reasoning for establishing the various requirements in this International Standard.

Aerosol drug delivery device design verification — Requirements and test methods

1 Scope

This International Standard applies to the design, labelling, instructions for use and testing requirements for hand-held single- and multi-use aerosol drug delivery devices (ADDDs) intended to deliver a metered or pre-metered aerosolized medication to or by means of the human respiratory tract (including nasal, oral, tracheal, bronchial and alveolar sites). This International Standard applies to both refillable and disposable devices intended for personal use.

This International Standard is intended for device design verification and not for drug product quality assessment. The objective of this International Standard is to verify, by laboratory (*in-vitro*) testing, that the ADDD design consistently meets the manufacturer's design specification by satisfying a device functionality profile and system verification test both of which are determined from a risk assessment and evaluated in accordance with the instructions for use.

This International Standard excludes continuous or semi-continuous aerosolization devices covered in ISO 27427, aerosolization devices which do not emit active pharmaceutical ingredient (API), general purpose aerosolization devices (for use with ventilators) and atomizers.

This International Standard does not apply to manufacturers of single parts or components of the ADDDs [e.g. (spray) pumps, valves, containers, etc.].

NOTE There might be times when a device falls under the scope of this International Standard and that of ISO 27427. The committee envisions that the intended use of the product and the risk assessment of the device will derive which International Standard the manufacturer chooses for design verification of the ADDD. This International Standard outlines the process by which ADDD design verification is to be performed in conjunction with a risk-based device functionality profile of the ADDD with either the medication, a placebo or a representative medication. ISO 27427 outlines the process by which the characterization of the aerodynamic aerosol performance of a nebulizing system for use with a non-specific class of active pharmaceutical ingredient(s) is made.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 14971:2007, *Medical devices — Application of risk management to medical devices*

ISO 10993-1, *Biological evaluation of medical devices — Part 1: Evaluation and testing*

ISO 11135-1, *Sterilization of health care products — Ethylene oxide — Part 1: Requirements for development, validation and routine control of a sterilization process for medical devices*

ISO 11137 (all parts), *Sterilization of health care products — Radiation*

ISO 15223-1, *Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied — Part 1: General requirements*